

COVID-19 Antigen Rapid Test Cassette (Anterior Nares)

Quick Reference Guide

NOTE:
Each test can be used **ONLY ONE TIME**. Do not try to use the test more than once.

Preparation

Test Pouch
(Test Device)



Extraction
Reagent



Collection
Tube



Sterile Swab




Disposable Gloves
(Not Provided)



Timer
(Not Provided)



Test Procedure

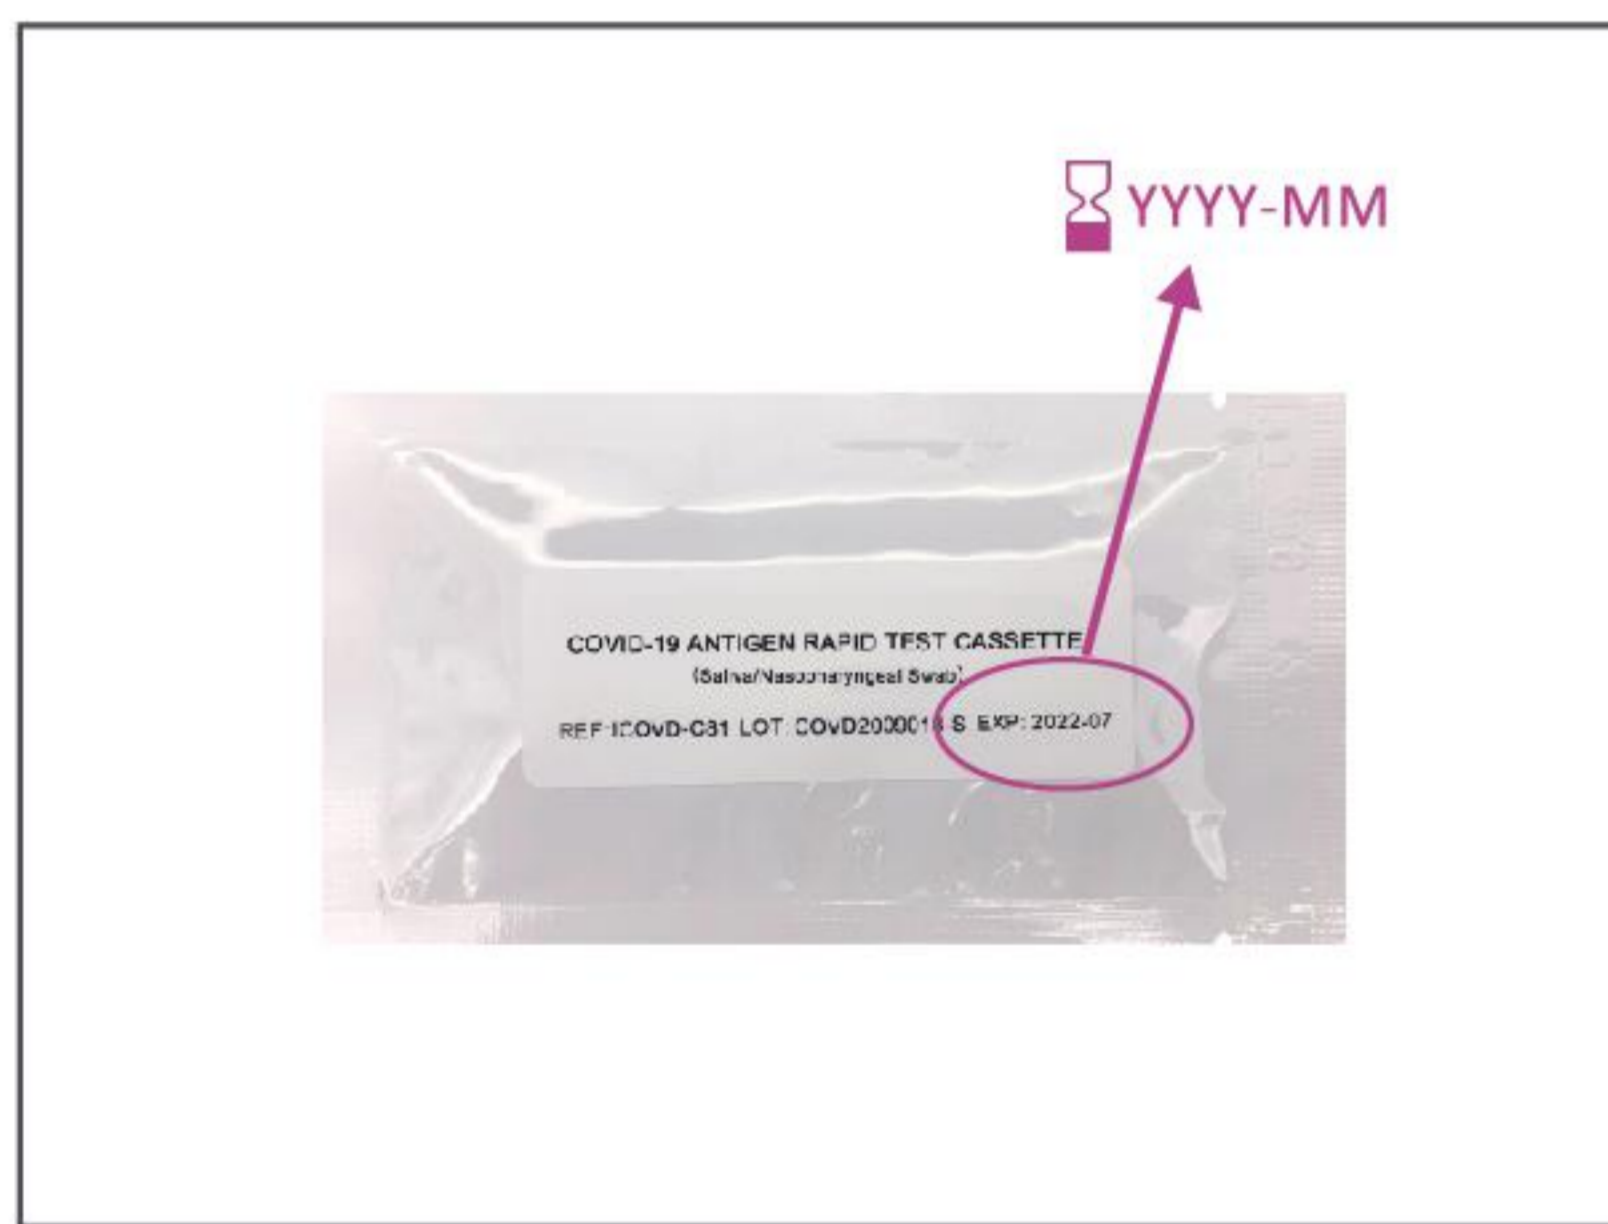


1. Check the expiry date. If expiry date has passed, use another kit.




2. Put on the gloves. Use new gloves for each patient.



3. Take out the collection tube.

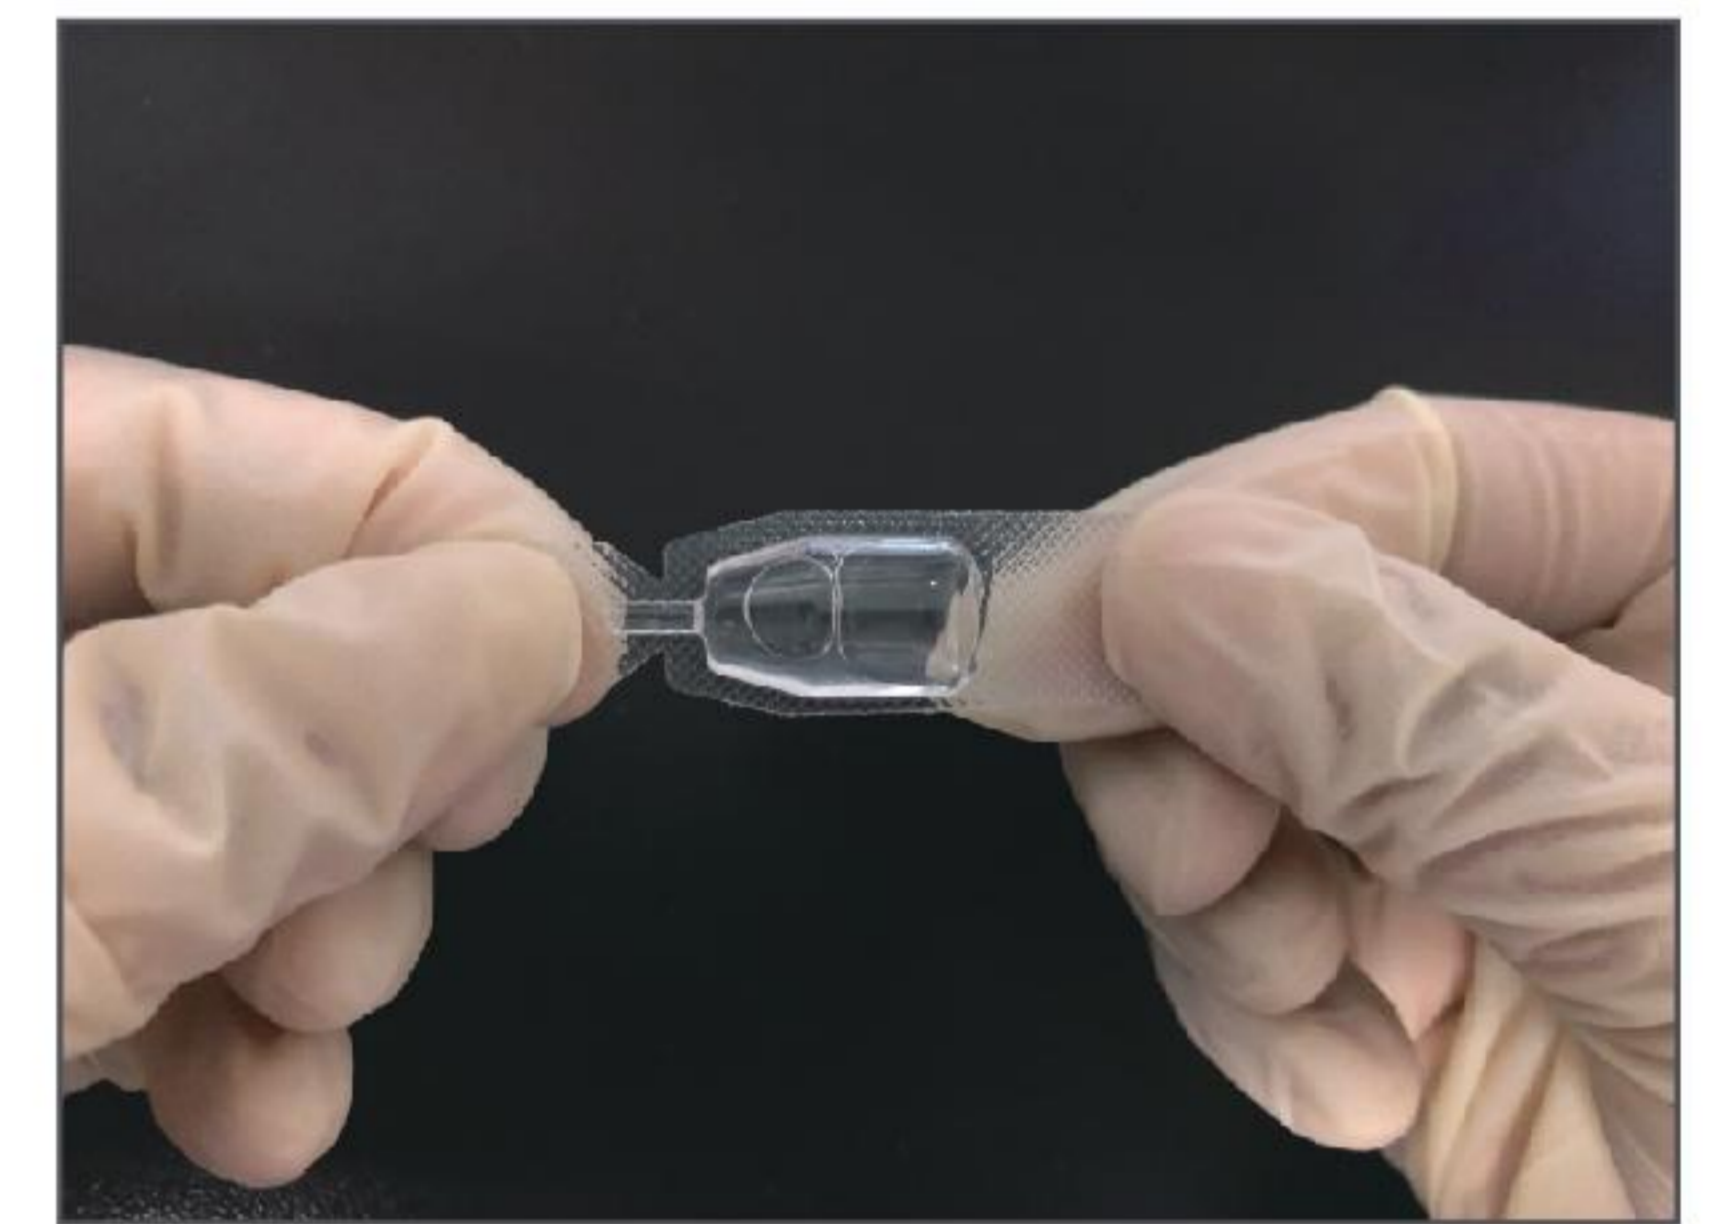


4. Twist the top off the extraction reagent bottle without squeezing.

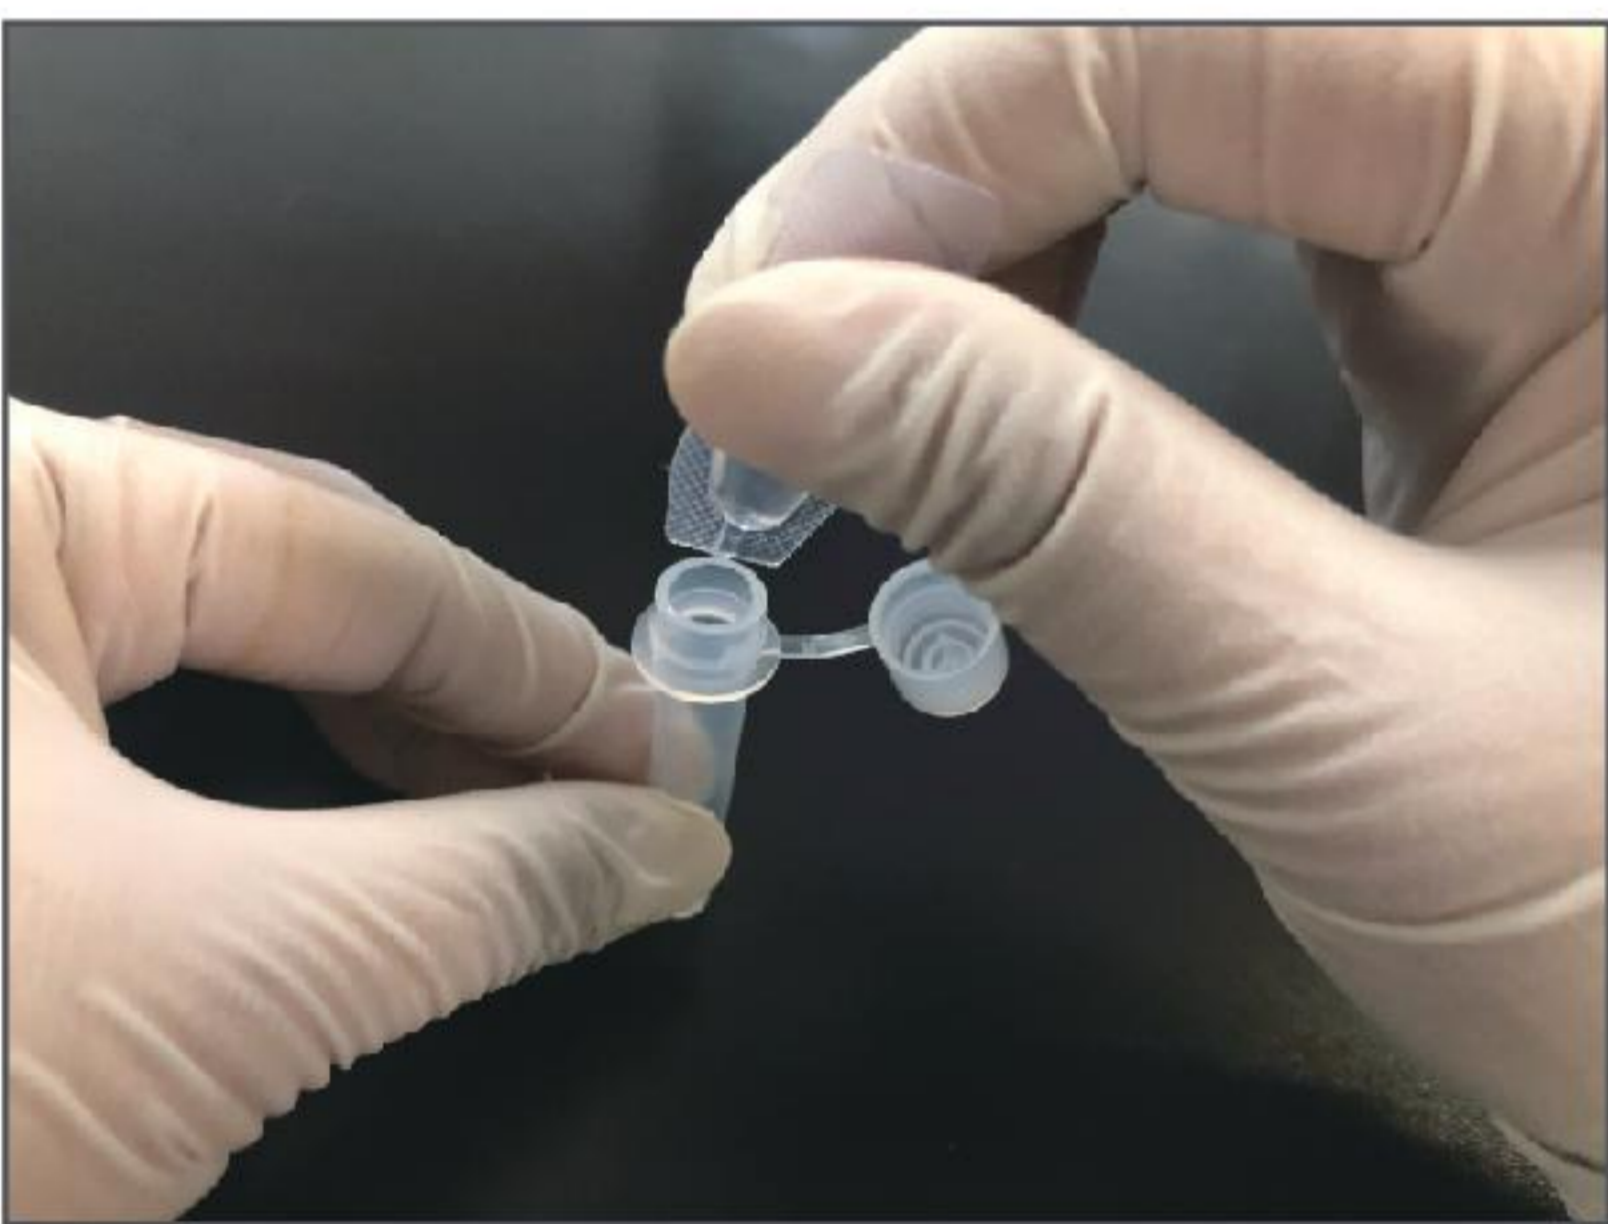


5. Add all the buffer to the collection tube.




6. Ask patient to blow their nose.

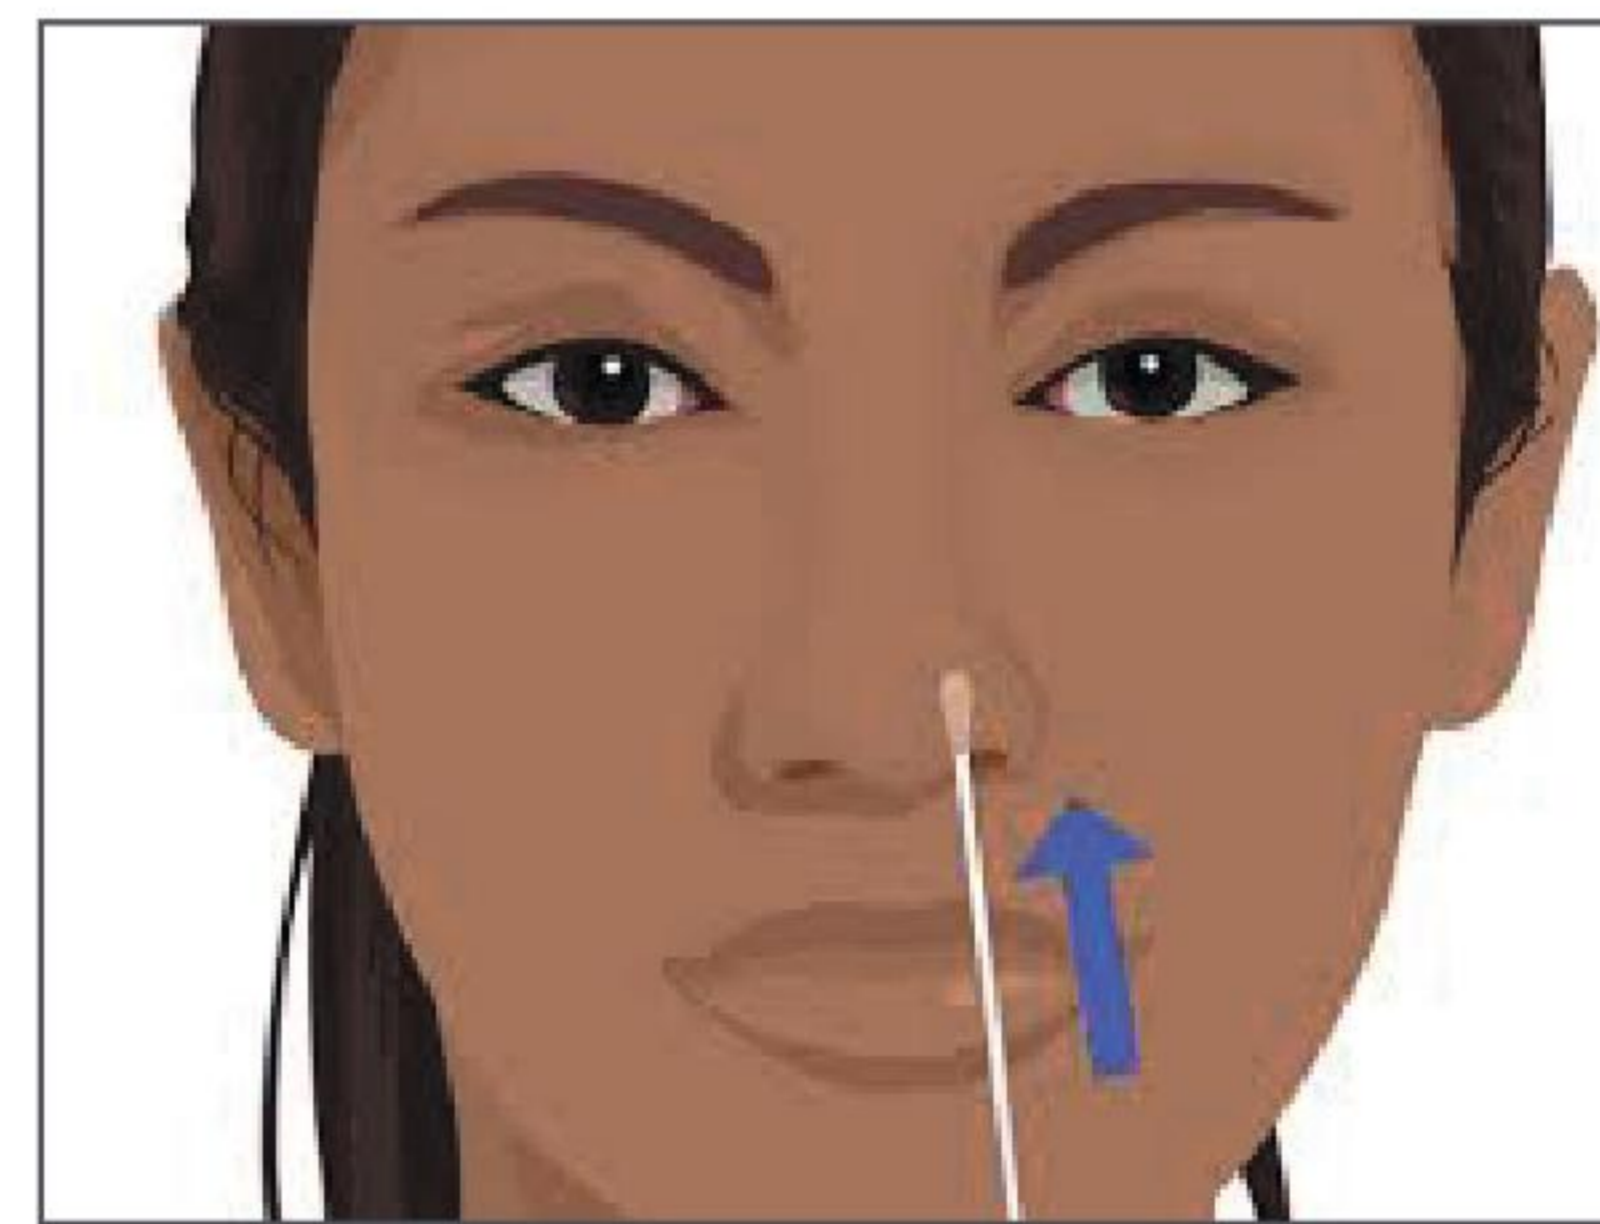


7. Insert a sterile swab into the anterior nares for 15 seconds for each nostril.

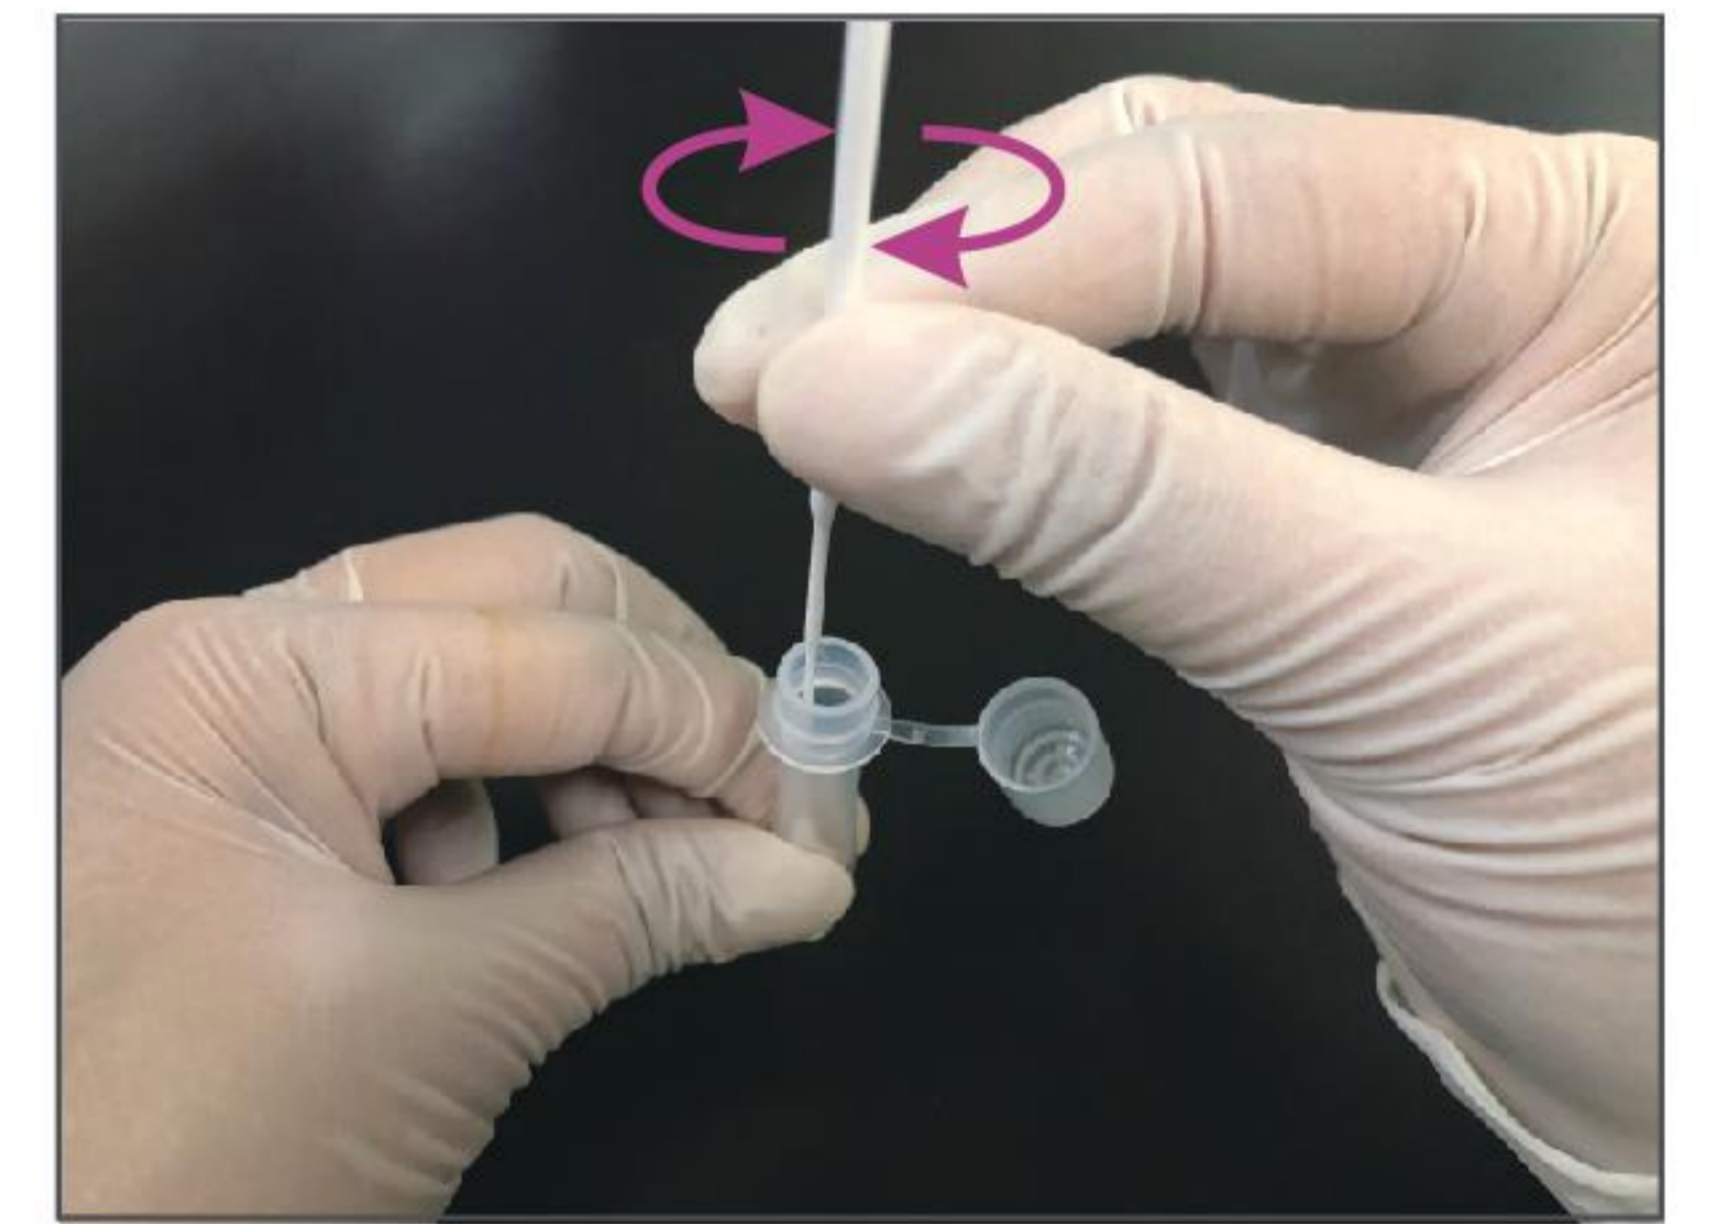

8. Place the swab into the buffer. Rotate the swab for 10 seconds while pressing the head against the inside of the tube.

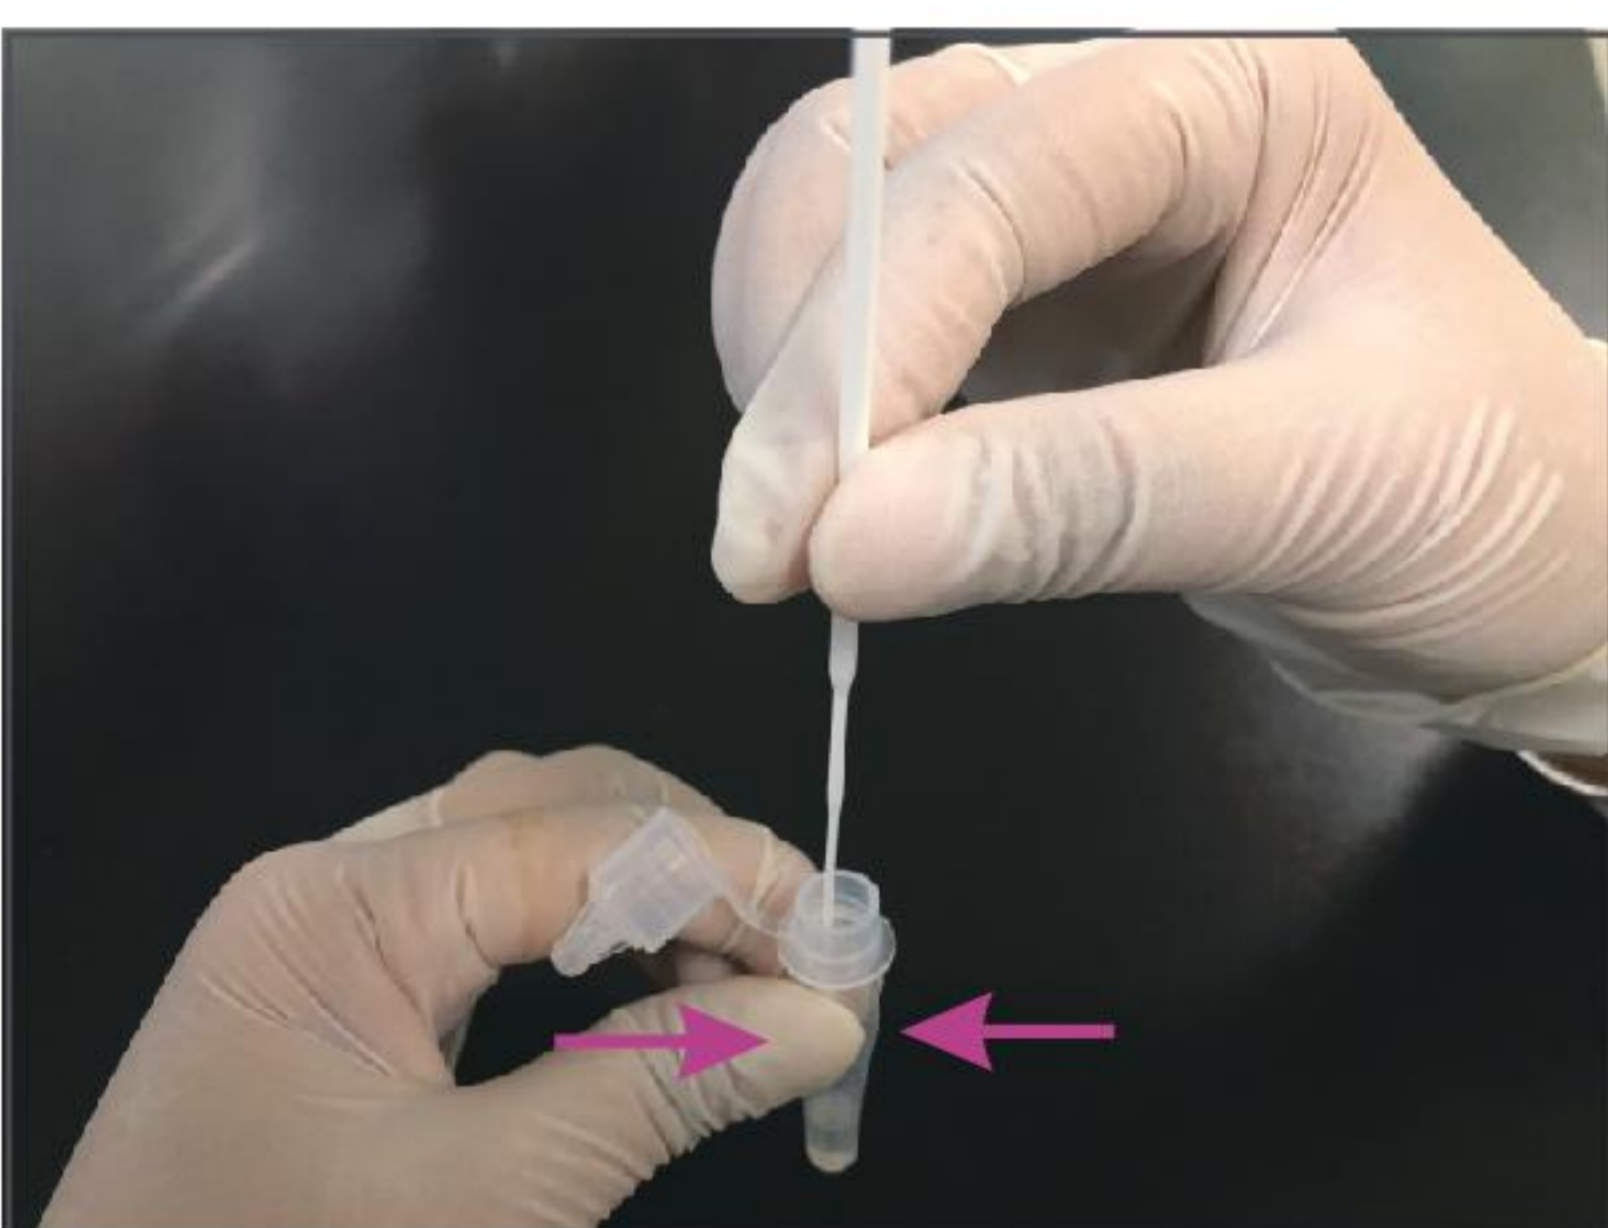

9. Remove the swab while squeezing the swab head against the inside of the tube.

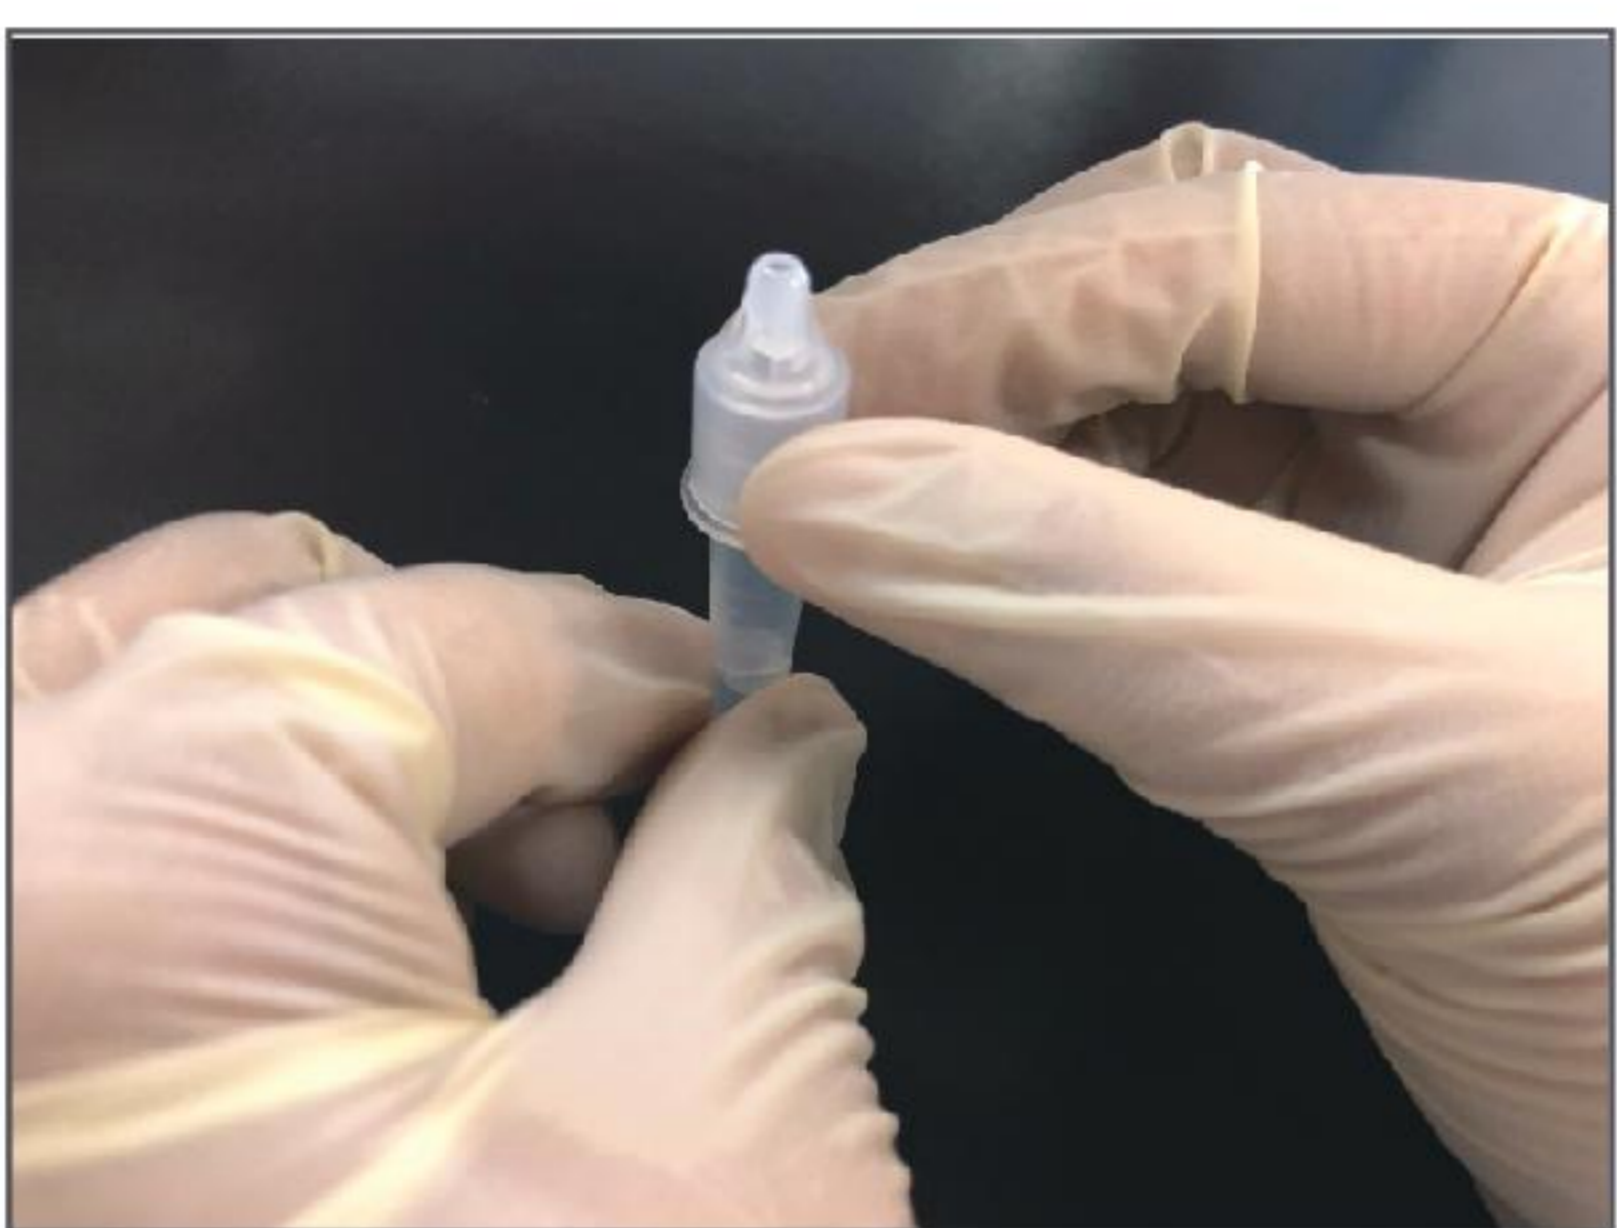

10. Close the lid.



11. Add 3 drops of the solution to the sample well.




12. Start timing and read result at 10 minutes. Do not interpret the result after 20 minutes.




All used tests, specimens and potentially contaminated materials should be discarded according to local regulations.

Overview

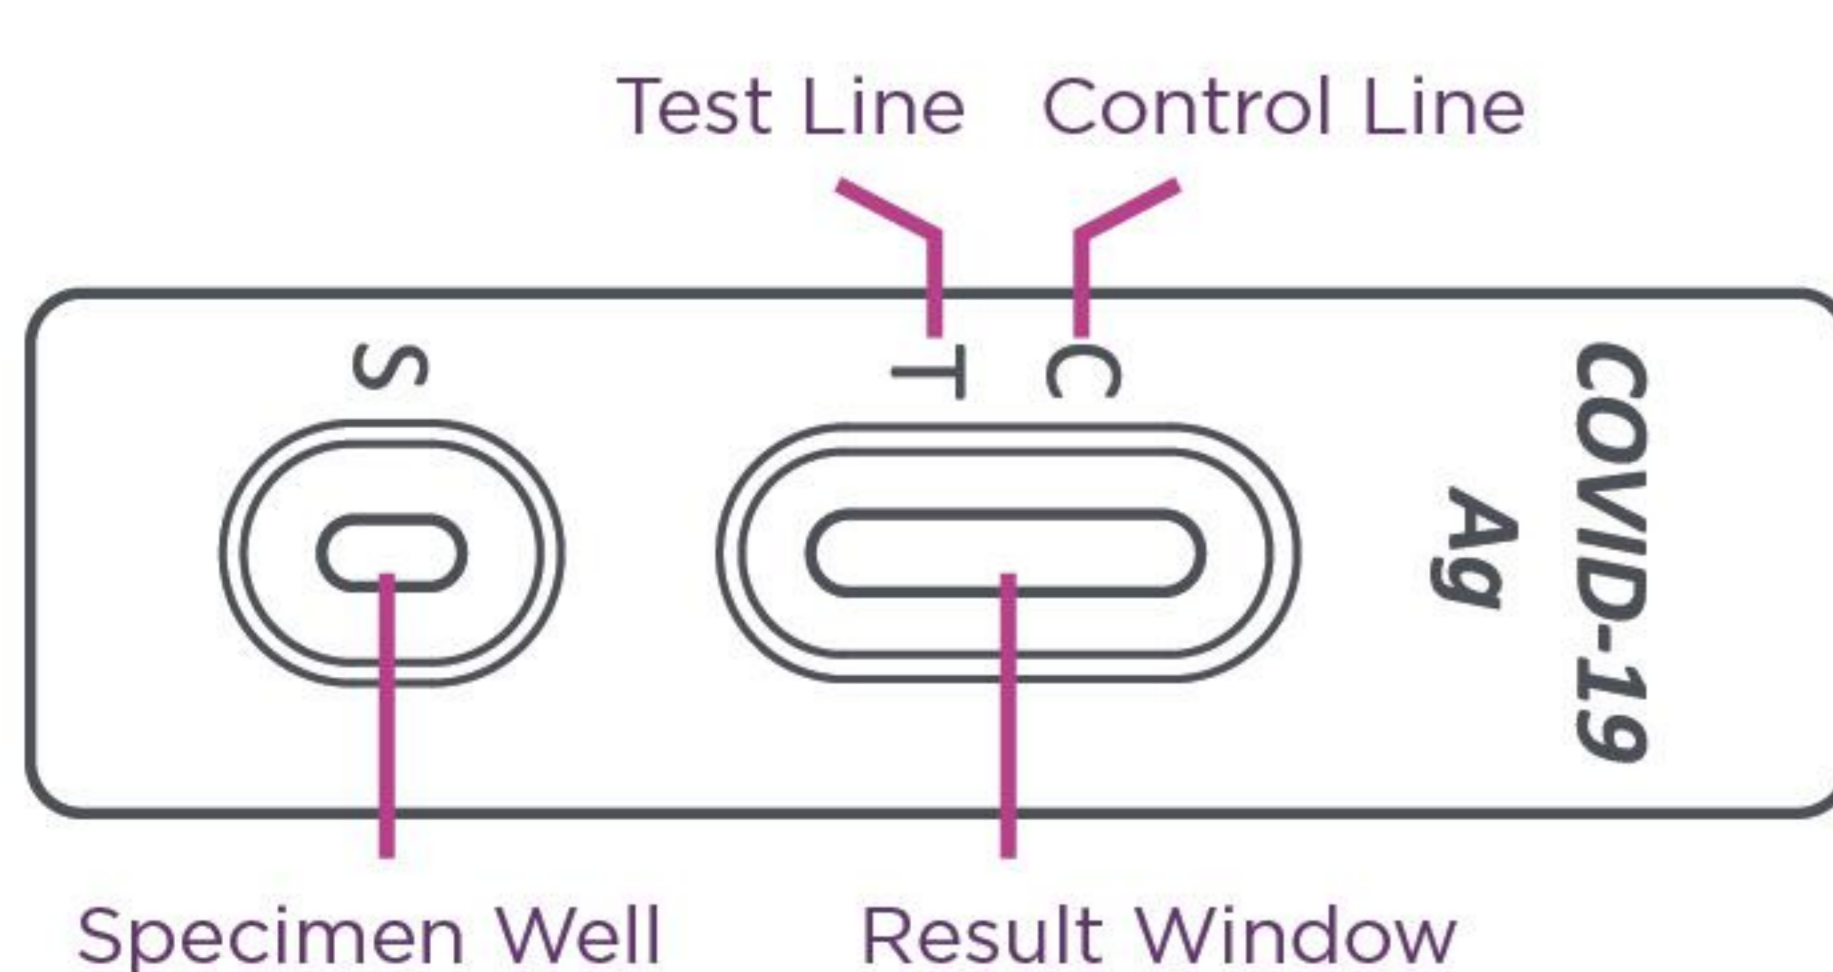


Interpreting Results

Positive

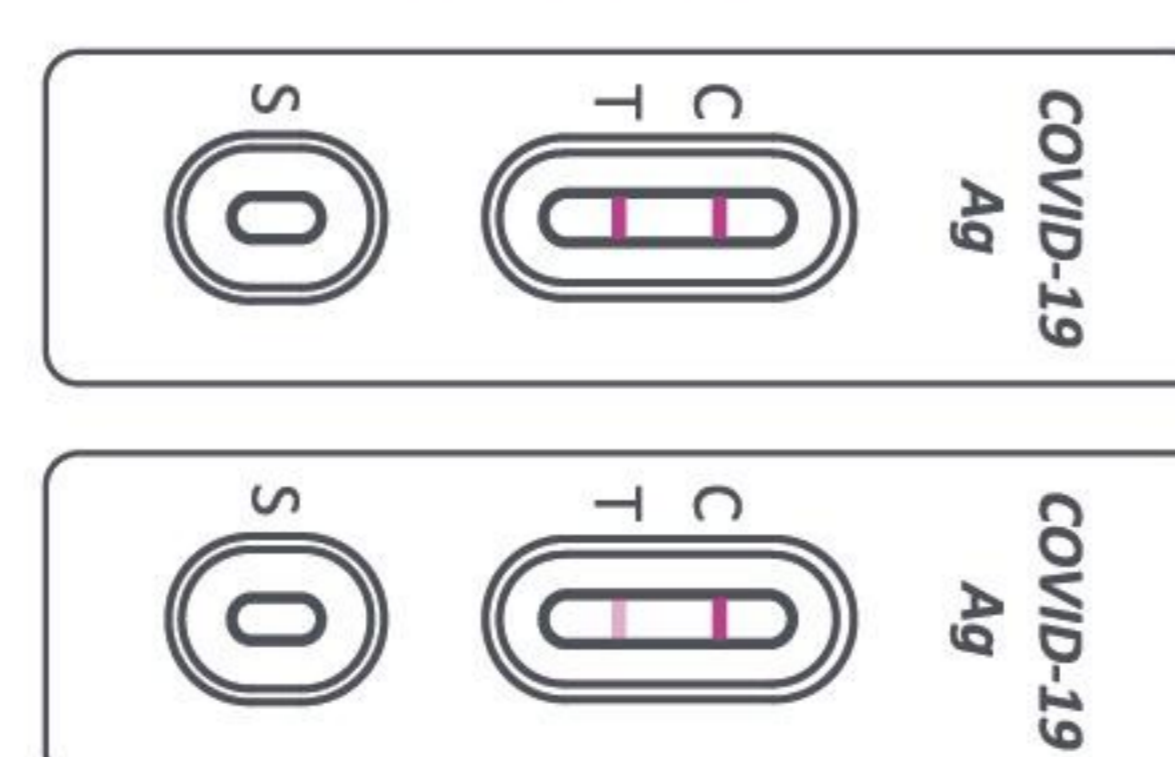


Two lines appear. One coloured line should be in the control line region (C) and another apparent coloured line should be in the test line region (T).

Negative

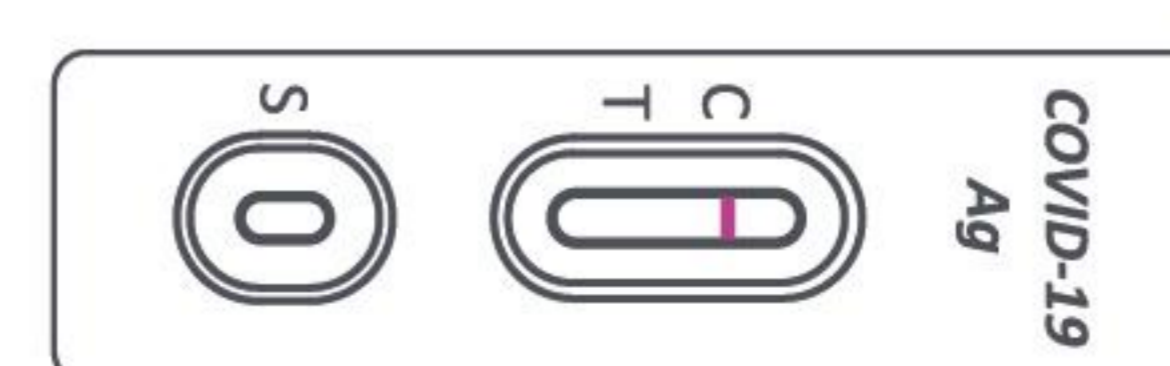

One coloured line appear in the control line region (C). No line appears in the test line region (T).

Invalid

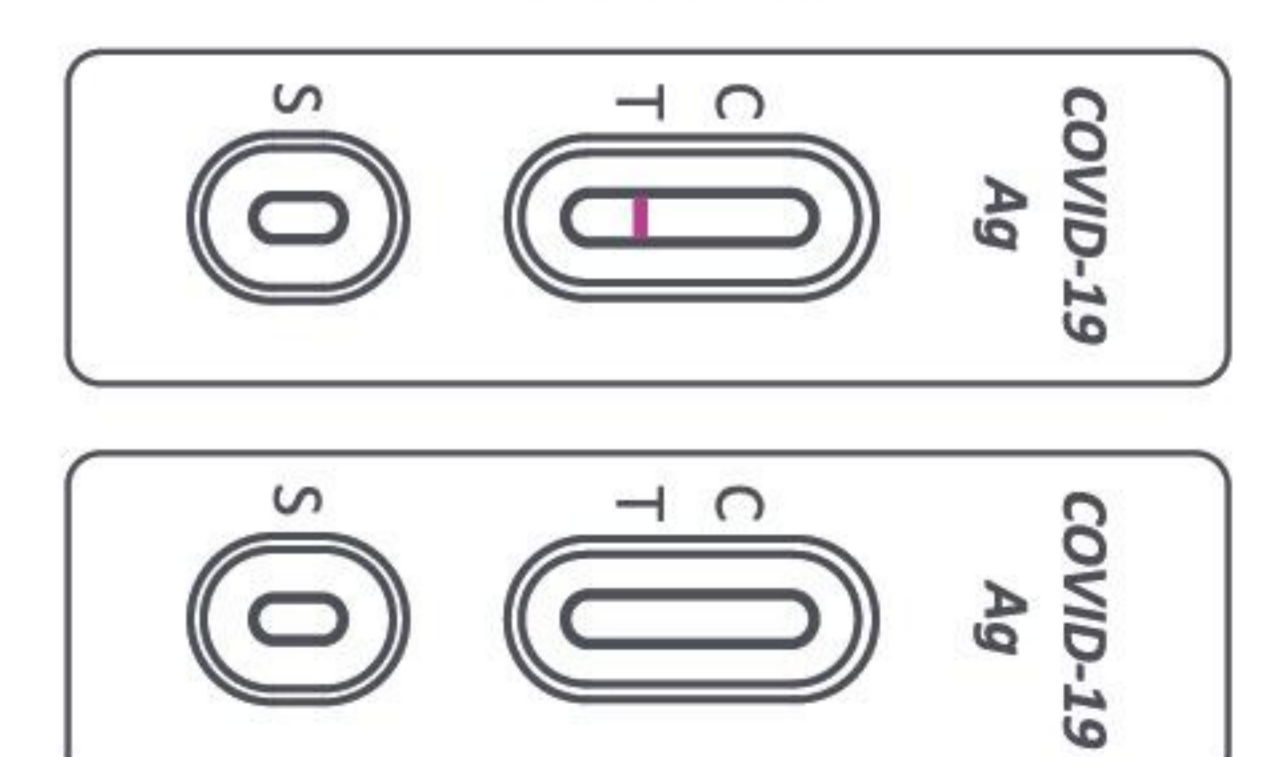

Control line fails to appear. Review the procedure and repeat the test with a new test.